


HIOKI



MEMORY HiLOGGER LR8431-20

Data Loggers

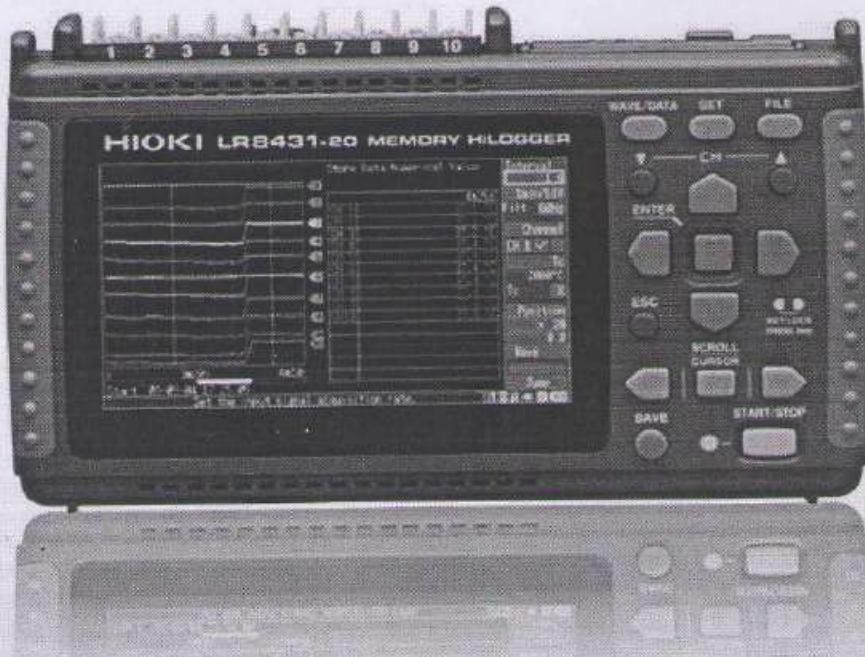

CE

Featuring USB flash drive support and improved accuracy


Your Personal 10-channel Logger



Real-time recording of up to 10ms/
sample data to USB or CF memory
devices



Small and light enough for the palm
of your hand - yet completely isolated

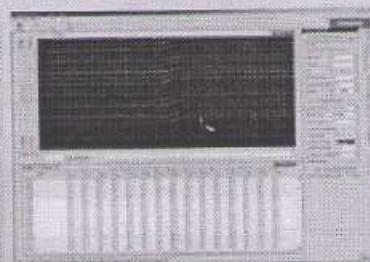

Logger Utility program supports
multi-channel measurements via PC



ISO 9001 ISO14001
JIS-C-0216 JCA-E-90201



IEC61010-1 certified devices, test products, measurement instruments
and other information is available on our website.

www.hioki.com

Lightest weight in its class and Easy Operation

Featuring USB flash drive support, faster performance, and more accurate thermocouple measurement



Redesigned to be even more capable, Hioki's 10-channel logger still fits in the palm of your hand.

■ ■ ■ **Ultra-compact for convenient portability**

Dimensions and mass (HiLOGGER only):
Approx. 176 mm (6.93 in) W × 101 mm (3.98 in) H × 41 mm (1.61 in) D, 550 g (19.4 oz)

■ ■ ■ **Provides ten electrically isolated analog input channels for measuring voltage and temperature, plus four pulse-counting input channels.**

The isolated inputs alleviate constraints while minimizing interchannel interference.

■ ■ ■ **10 ms scanning of all channels provides rapid sampling capabilities**

Track waveforms to meet demands for measuring sudden changes in loads

■ ■ ■ **Widescreen, bright LCD gives excellent viewability**

The beautiful, wide QVGA-TFT display is ideal for waveform monitoring.

■ ■ ■ **Featuring USB flash drive support**



The LR8431-20 can record measurement data on a USB flash drive for easy transfer to a computer. In long-term measurement applications, it can also record to reliable Compact Flash cards for increased peace of mind.

1

Replace storage media during real-time recording

Switch out fully loaded storage media with new ones while recording without stopping the measurement so that you can analyze any data recorded so far.

Note: During high-speed recording, be sure to insert the new storage media within 2 minutes of removing the former.

2

Display remaining recording time

The LR8431-20 lets you check the remaining recording time based on the available capacity on your CF card or USB flash drive.



Savable
time : USB
26d

Setting screen

3

Load data from previous MEMORY HILOGGER 8430-20 models

The LR8431-20 can also load waveform and settings data from previous MEMORY HILOGGER 8430-20 models, allowing it to make measurements using the same settings and display past data.

4

Copy data between storage media


The LR8431-20 can copy recorded data between the CF card and USB flash drive.

Use only HIOKI CF cards, which are manufactured to strict industrial standards, for long-term storage of important data. Operation of non-HIOKI CF cards is not guaranteed.

■ ■ ■ **The LR8431-20 delivers Improved thermocouple measurement accuracy and reference junction compensation accuracy.**

Example: When measuring 50°C water with a type-K thermocouple
The LR8431-20 provides improved accuracy of $\pm 1.5^{\circ}\text{C}$, whereas previous models provided accuracy of $\pm 3^{\circ}\text{C}$.

50°C

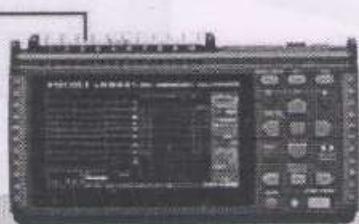

Improved Accuracy!

Previous
MEMORY HILOGGER
(8430-20)
 $\pm 3^{\circ}\text{C}$

LR8431-20
Accuracy

$\pm 1.5^{\circ}\text{C}$

Measurement Accuracy: $\pm 2^{\circ}\text{C}$
Reference junction compensation accuracy: $\pm 1^{\circ}\text{C}$

Measurement Accuracy: $\pm 1^{\circ}\text{C}$
Reference junction compensation accuracy: $\pm 0.5^{\circ}\text{C}$

Evaluating motors and inverters used in electric and hybrid vehicles

The LR8431-20 enables stable, low-noise measurement of high-speed, high-resistance targets.

Efficiency measurement and performance evaluation of air conditioning equipment

The LR8431-20 supports simultaneous, multi-point measurement, for example of input and output at multiple air conditioning registers or the temperature of internal components.

Temperature measurement and performance evaluation of internal components in electronic equipment

Used with a wind velocity converter, the LR8431-20 can measure cooling efficiency inside equipment enclosures.



Isolated
10ms
10ch

This compact logger excels in a broad range of settings, from production lines to research and development.



Ten Isolated Analog Input Channels

There's no need to worry about differing potentials of measurement objects when measuring temperature and voltage. All ten analog channels are isolated.


Even when measuring temperature and voltage at the same time, interchannel interference and electric shock hazards are eliminated. The four pulse channels are ideal for counting revolution pulses to measure rotation speed.
Note: Pulse inputs share common ground.



High-Speed Sampling

10 ms Sampling and Recording Across All Channels

Abrupt changes in load need to be measured during development of EV・HV・PHV, for which multi-channel, 10 ms sampling is essential. This HILOGGER can track waveforms that could not be followed with the 100 ms sampling interval previously available.

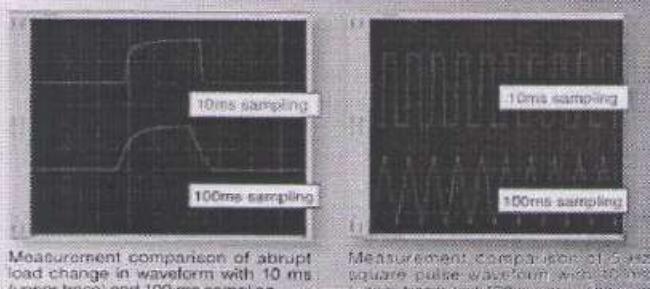

(using the supplied Logger Utility program)




Enhanced Noise Suppression

Noise-resistant measurement circuitry for improved readings

Measurement involves the deployment of a delta-sigma type A/D converter. Suppress inverter switching noise and line-frequency hum by digital filtering with the HILOGGER's proprietary oversampling technology.

Note: Optimum noise suppression is obtained for recordings at least two seconds long.

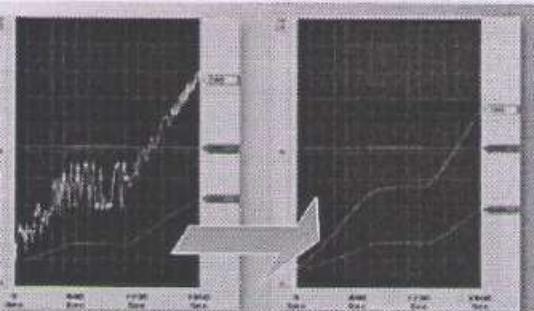


(using the supplied Logger Utility program)

Collect data in real-time with a computer **Logger Utility** (Accessory)

The LR8431-20 ships standard with Logger Utility, a software application that supports multi-channel computer measurement. Simply connect the logger to a computer with a USB cable.


■ ■ ■ USB connection ensures easy setup

Configure Hi.LOGGER settings from the Logger Utility. Settings are sequentially ordered and guided from the PC application.

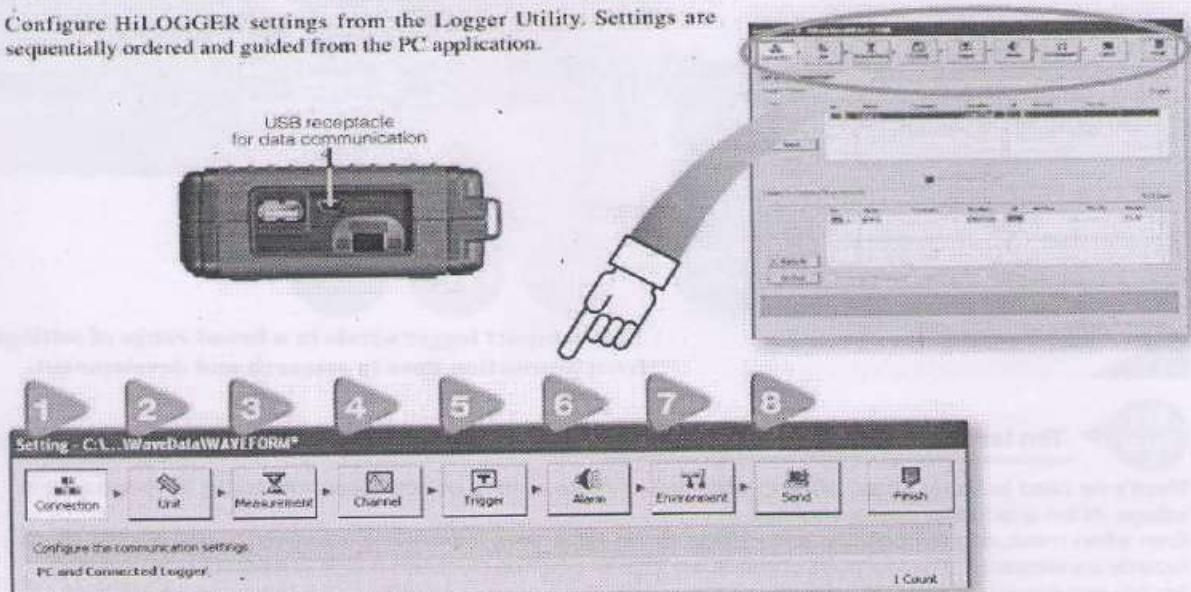


Up to five LR8431-20 instruments can be connected to a single computer with USB cables.

Providing 50 analog and 20 pulse channels that can be graphically displayed together in one window.

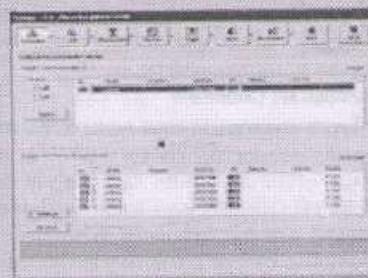


■ USB cable connection

A USB hub can be used to enable multi-channel measurement of multiple locations.

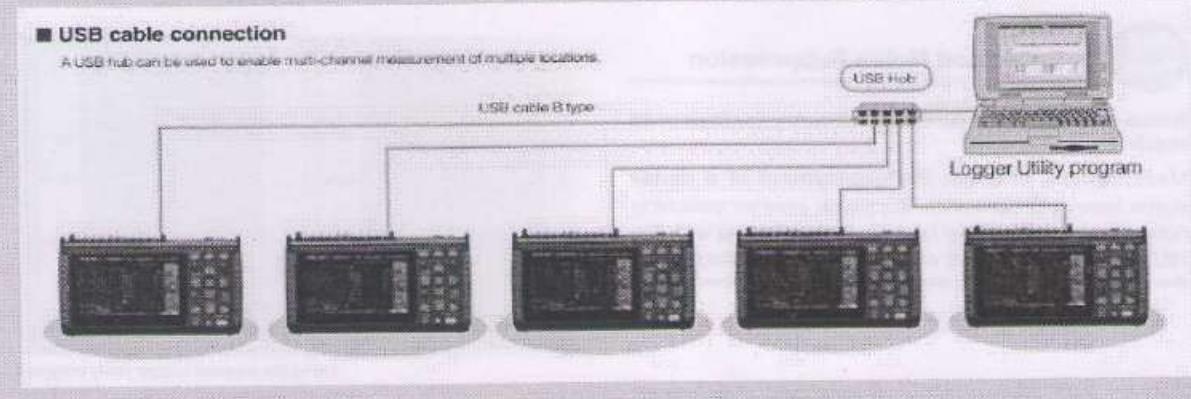

Collect data in real-time with a computer **Logger Utility** (Accessory)

Control measurements from the PC screen

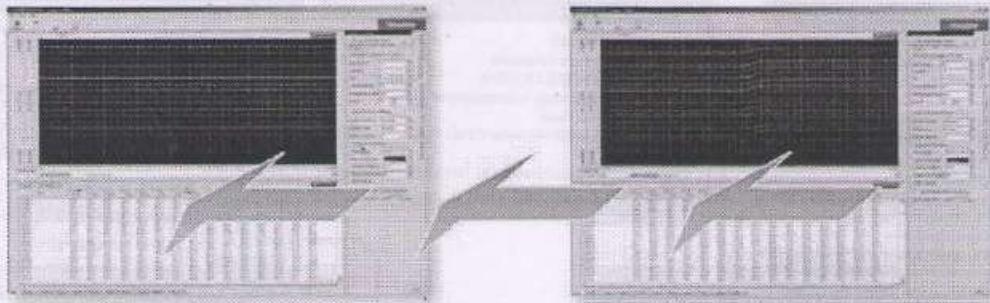

Use the supplied Logger Utility program to control real-time data recording from the PC. Scroll backward through the displayed trend graph window to view past waveforms even while recording.


Up to five LR8431-20 HiLOGGERS can be connected to one PC, providing 50 analog and 20 pulse channels that can be graphically displayed together in one window.

Patented "dual-knob function"

You can use the scrollbar to confirm what the position of the waveform portion displayed on the screen is within the whole recorded waveform.

The ability to change the time axis shown on individual windows provides a convenient way to analyze data collected over an extended period of time.

*Analysis using the dual-knob function is a patented Hioki technology.

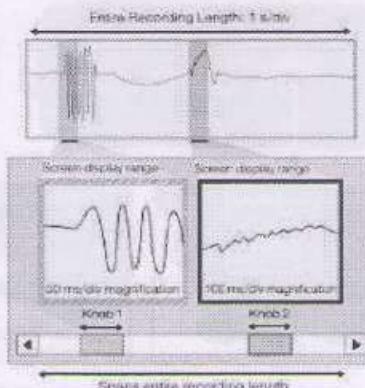


■ Logger Utility (bundled application software)

Operating environment	One CD-R, CPU: Pentium 3 (500 MHz or more), at least 512 MB of memory Interface: USB (LAN not available with the Model LR8431-20) OS: Windows 7 (32-bit, 64-bit), Vista (32-bit, 64-bit), Win 7.50 or later /XP SP2 or later, Windows 2000 SP4 or later (This software is compatible only with the MEMORY HiLOGGER LR8431-20, LR8400-20s, LR8400-21s, 8423, 8430-20/21)	Data conversion Target data: Real-time data acquisition file (LUW format). Record to internal memory data (MEM format). Waveform processing data Converted sections: All data, designation section Format: CSV format (separate by comma, space, tab), transfer to EXCEL spreadsheet; arbitrary data thinning
Real-time data acquisition	Measurements on multiple loggers connected by USB can be controlled to sequentially acquire, display and save waveform data for recording up to 10 million samples *LAN not available with the Model LR8431-20	Parameter calculations Number of controllable instruments: up to 5 units Display: Waveforms (multiple time axis) can be displayed; Numerical values (logging); Alarm status at the same time; Numerical value monitoring in a separate window. Waveforms scroll while measuring Data saving destination: Real-time data transfer to EXCEL (new function), or Real-time data acquisition file (LUW format, only for HiOKI Event marks) can be applied while recording
Data acquisition settings	Data acquisition settings for the HiLOGGER Saving: The setting for multiple HiLOGGERS can be saved together in one file (LES format). Instrument configuration settings can be sent and received	Search function Target data: Real-time data acquisition file (LUW format). Record to internal memory data (MEM format). Waveform processing data Search mode: event mark, time and date, maximum position, minimum position, maximum pole, minimum pole, alarm position level, window, amount of change
Waveform display	Processed data file: Real-time data acquisition file (LUW format). Record to internal memory data (MEM format) Display format: Simultaneously display waveform and numerical value, time-axis divided display possible Maximum number of channels: 50 channels (measurement data, used with the LR8431-20s + 60 channels (waveform processing data)) Others: Waveform display on sheet for each channel, scroll, record event mark, cursor, hard copy, numerical value display	Print function Supported printer: printer compatible with the OS Target data: Real-time data acquisition file (LUW format). Record to internal memory data (MEM format). Waveform processing data Print format: waveform image, report format, list print (channel settings, event cursor value) Print area: the entire area, area between cursors A and B Print preview: supported
		Waveform processing Processing items: Four arithmetic operations Number of processing channels: 60 channels

■ ■ ■ Functionality

- ▶ A variety of transducer outputs (DC voltage), or thermocouple measurements over 10 channels
- ▶ 4 Pulse (count) Input Channels, 1 Alarm Output Channel
- ▶ Real-time Save & Long-term recording to CF Card or USB memory

For more reliable data protection, we recommend use of HIOKI CF cards, which are manufactured to strict industrial standards, for real-time saving of data or long term storage of important data. The USB communications function cannot be used while saving data to a USB flash drive. Operation of non-HIOKI CF cards is not guaranteed.

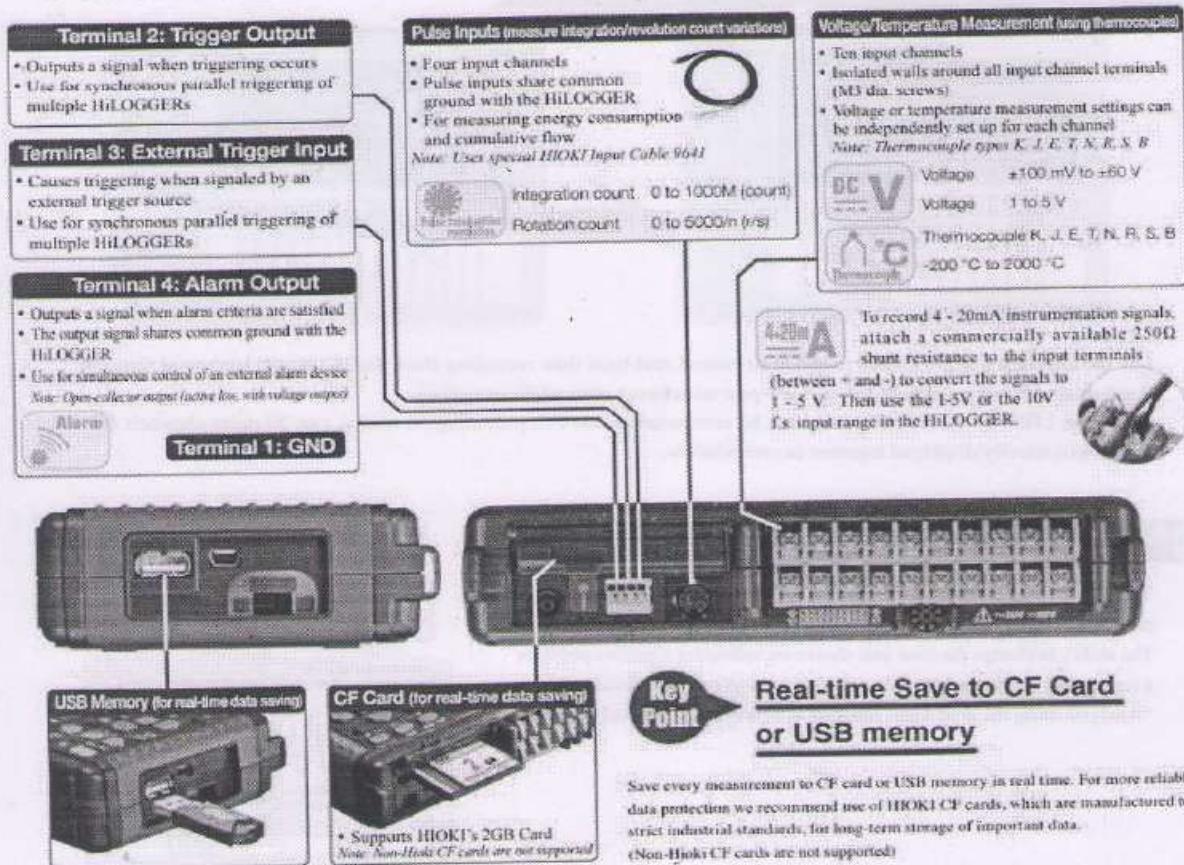

Recording Time (Save to External storage in real-time of binary data) *Note: When saving in CSV data format, total recording time is 1/10 of those of the following*

Recording intervals	Internal memory (7 MB)	Recording All Channels (analog, four pulse and one alarm)			
		256 MB	512 MB	1 GB	2 GB
10 ms	32m	19h 37m	1d 15h 14m	3d 06h 29m	6d 12h 58m
20 ms	1h 04m	1d 15h 14m	3d 06h 29m	6d 12h 58m	13d 01h 57m
50 ms	2h 40m	4d 02h 6m	8d 04h 13m	16d 08h 26m	32d 16h 53m
100 ms	5h 21m	8d 04h 13m	16d 08h 26m	32d 16h 53m	65d 09h 47m
200 ms	10h 43m	16d 08h 26m	32d 14h 53m	65d 09h 47m	130d 19h 35m
500 ms	1d 02h 49m	40d 21h 07m	81d 18h 14m	163d 12h 29m	325d 00h 59m
1 s	2d 05h 39m	81d 18h 14m	163d 12h 29m	327d 00h 59m	"★"
2 s	4d 11h 18m	163d 12h 29m	327d 00h 59m	"★"	"★"
5 s	1d 04h 16m	"★"	"★"	"★"	"★"
10 s	22d 08h 33m	"★"	"★"	"★"	"★"
20 s	44d 17h 06m	"★"	"★"	"★"	"★"
30 s	67d 01h 39m	"★"	"★"	"★"	"★"
1 min	134d 03h 18m	"★"	"★"	"★"	"★"
2 min	268d 06h 36m	"★"	"★"	"★"	"★"
5 min to 1 hour	"★"	"★"	"★"	"★"	"★"

* Maximum recording time is inversely proportional to number of recording channels.

* Because the actual capacity of the External storage is less than that indicated, and because the header portion of waveform files is not included in capacity calculations, expected actual recording times to be about 90% of those in this table.

* * Exceeds 365 days.

■ Product Specifications

General specifications (product guaranteed for one year)		Measurement Settings	
Input System/ Channels	<p>Analog inputs: 10 (M3 mm dia. screw terminal block), electrically isolated between channels, and from chassis ground.</p> <p>Input impedance: 1 MΩ (when voltage input or temperature measuring with thermocouple burn-out detection OFF), 800 kΩ (with thermocouple burn-out detection ON)</p> <p>Pulse inputs: 4 channels (requires HIOKI Input Cable 9641)</p> <p>Note: all pulse inputs share common ground with the HiLOGGER</p>	Recording Intervals (Sampling period) 10 ms to 1 hour, 19 selections Note: All input channels are scanned at high speed during every recording interval	
Analog Inputs	<p>Maximum rating: 60 V DC (max. voltage between input terminals without damage)</p> <p>Maximum rated voltage from isolated terminals to ground: 60 V DC (max. voltage between input channel terminals, and from terminals to chassis ground without damage)</p>	Graph Timebase Scaling 100 ms to 1 day per division, 21 selections Note: Setting is independent from the recording interval	
Pulse Inputs	<p>Input limits: -5 to +10 V DC (max. voltage between input terminals without damage), non-isolated (common ground between pulse input channels, and with chassis)</p> <p>Pulse signal characteristic: No-voltage relay contact "a", open collector or voltage input (High: ≥ 2.5 V, Low: ≤ 0.9 V), Period: at least 200 µs (both high and low periods at least 100 µs)</p>	Repeating Recording (ON/OFF) Enable to repeat recording after the specified recording time span has elapsed	
Alarm Output	<p>One channel, non-isolated: output from external control connector (common ground)</p> <p>Signal criteria: configurable high/low threshold levels, enter/exit threshold window, logical sum (OR) and logical product (AND) for every input channel. Output is refreshed each time recording starts.</p> <p>Signal characteristic: Open-collector output (active low, with voltage output)</p> <p>Voltage levels: 4.0 to 5.0 V (H) and 0 to 0.5 V (L), Max. sink current: 5 mA DC, Max. applied voltage: 30 V DC</p>	Recording Time Enable continuous recording ON (records until the Stop key is pressed), or disable to record for a specified time span (days, hours, minutes and seconds)	
Internal storage	3.5 MWords (7 MB of two-byte data points, or four-byte pulse measurements)	Timer Recording (ON/OFF) Enable to record for a specified time span, or between specified start and stop times	
External storage	<p>CF card: CF card slot × 1, HIOKI 9727 (256 MB), 9728 (512 MB), 9729 (1 GB), 9830 (2 GB). Data format: FAT, FAT32</p> <p>USB memory: USB 2.0 High-speed capable, series mini-B receptacle, Data format: FAT, FAT32</p>	Auto Saving Waveform (Binary or CSV data): stores data to the CF card or USB memory during real-time measurement	
Backup Function (@15°C)	Backup battery life for clock and settings: approx. 5 years For measurement data: 100 hours with fully charged battery pack, or for as long as AC adapter is connected	Numerical value calculations: stores calculated values to the CF card or USB memory when finished measuring Note: Don't shutdown while data saving	
External Control Terminals	External Trigger/Event Mark input (exclusion function), Trigger Output, Alarm Output	Data Storage Methods Each recording can be saved in a separate file Overwriting save (endless loop recording): New data overwrites the oldest data when the storage media is full	
Display type	4.3-inch WVGA-TFT color LCD (480 × 272 dots)	Divided Saving: Enable to save data at a specified interval (days, hours and minutes) Divided Saving: Specified Time (specify a time of day at which to start saving data to files at a specified interval) Note: Don't shutdown while data saving	
Displayable languages	English, Japanese	Load Stored Data Stored data can be recalled by the HiLOGGER in 3.5 MWord (7 MB) quantities (for a single channel; less for multiple channels)	
External Interface	One USB 2.0 series mini B receptacle Functions: Control from a PC (Ver 1.00 or later), Transfers internal data on the CF card to a PC	Settable Save/ Reload Configure saving and reloading to and from CF card or USB memory or internal memory	
Environmental conditions (no condensation)	<p>Temperature and humidity range for use: 0°C to 40°C (32°F to 104°F), (or 5°C to 30°C, 41°F to 86°F when battery charging), 80% rh or less</p> <p>Temperature and humidity range for storage: -10°C to 50°C (14°F to 122°F), 80% rh or less</p>	Numerical Calculations Ten types for internal memory, no limit for CF card and USB memory	
Compliance standard	Safety: EN61010, EMC: EN61326, EN61000	Selectable Filters Calculations 1 to 4, may be simultaneous	
Power Sources	<p>(1) 100 to 240 V AC, 50/60 Hz using AC ADAPTER Z1005 (2) BATTERY PACK 9780 (when used with the AC Adapter, the AC Adapter has priority)</p> <p>(3) 12 V battery (10 to 16 V DC ±10%. Please contact HIOKI for connection cord)</p>	Alarm output (I): Hold/not-hold, beeper enable/disable (ON/OFF), Show/hide alarm waveform display (ON/OFF)	
Power Consumption	10 VA	Channel Settings	
Continuous Operating Time	Approx. 2.5 hours (with Battery Pack Model 9780 while saving to the CF card)	Channel Settings	Enable/disable measurement (ON/OFF), selectable waveform color
	Charging time: Approx. 200 minutes (@5°C to 30°C ambient)		Analog channels (10): Voltage (DC only), Temperature (thermocouple only), Thermocouple types K, J, E, T, N, R, S, B
Dimensions and mass	Approx. 176 mm (6.93 in) W × 101 mm (3.98 in) H × 41 mm (1.61 in) D, 550 g (19.4 oz) (HiLOGGER only)		Pulse input channels (4): Count integration or revolutions
Supplied Accessories	Measurement Guide × 1, AC ADAPTER Z1005 × 1, USB cable × 1, CD-R (Instruction Manual, data collection software "Logger Utility") × 1		Alarm output (I): Hold/not-hold, beeper enable/disable (ON/OFF), Show/hide alarm waveform display (ON/OFF)

Trigger functions

Trigger Source (selectable for each channel)	All analog and pulse channels P1 to P4, external trigger, logical sum (OR) and product (AND) of each trigger source	Temperature Other Functions	Thermocouple burn-out detection: ON or OFF
External Trigger	Criteria: Short-circuit between external trigger input and ground, or voltage input (H-L transition from [3.0 – 5 V] to [0 – 0.8 V]) Pulse width: At least 1 ms (H), and 2 µs (L) Input limits: 0 to 7 V DC	Measurement parameters	Ranges Range of Measurements Finest Resolution
Trigger Timing	Start, Stop and Start/Stop (different trigger criteria can be set to start and stop)	Pulse (Totalization)	1,000 M (count) f.s. 0 to 1,000 M (count) 1 (count)
Trigger Types (Analog, Pulse)	Level: Triggers when rising or falling through preset threshold Window: Triggers when entering or exiting range defined by preset upper and lower thresholds		Totalization mode: cumulative (counts from start) Instantaneous value: instantaneous value during each recording period
Level Resolution	Analog: 0.025%/f.s. (f.s. = 10 display divisions) Pulse: Totalization 1 count, Rotations 1/n [f.s.] (n: pulses per rotation)	Pulse (Rotations)	5,000/n (r/s) f.s. 0 to 5,000/n (r/s) 1/n (r/s)
Pre-trigger	Records for a specified period before triggering; can be set for real-time saving	Slope Setting	Settable pulses per rotation: 1 to 1,000 ("n" above is the number of sensor output pulses per rotation)
Trigger Output	(1) Output signal at trigger occurred, (2) Output signal at start or trigger occurred, (1) or (2) mode selectable Open collector (active low, with voltage output, at least 10 ms pulse width, Voltage levels: 4.0 to 5.0 V (H) and 0 to 0.5 V (L), Max. sink current: 5 mA DC, Max. applied voltage: 30 V DC)	Displayed Range	↑ (count of L-to-H pulse transitions), ↓ (count of H-to-L pulse transitions) Specified by position, or by upper/lower display limit values (Upper/lower limit values only at Totalization mode)
		Common Channel Settings	Decimal (display decimal values), Exponential (display base-10 exponents), or Off
		Scaling	Method: Ratio (set by slope and intercept), or 2-point (set by input/output values at two points)
		Other Common Channel Settings	Enter comments for each channel, set start/stop triggers and alarm criteria

■ Options in Detail



MEMORY HILOGGER LR8431-20 (English model)

Supplied Accessories:

Measurement Guide × 1, AC ADAPTER Z1005 × 1, USB cable × 1,
CD-R (instruction Manual, data collection software "Logger Utility") × 1



AC ADAPTER Z1005
100 to 240 V AC



Supplied with
PC Card adapter

PC Card Precaution

Use only PC Cards sold by HIOKI. Compatibility and performance are not guaranteed for PC cards made by other manufacturers. You may be unable to read from or save data to such cards.

PC CARD 2G 9830 (2 GB capacity)

PC CARD 1G 9729 (1 GB capacity)

PC CARD 512M 9728 (512 MB capacity)

PC CARD 256M 9727 (256 MB capacity)



Charger while installed
in the HILOGGER

BATTERY PACK 9780
NiMH. Charge while installed



CONNECTION CABLE 9641
For pulse inputs, 1.5 m (4.92 ft) length




To prevent damage to
the instrument's display
For LCD protection, pairs of additional sheets
can be purchased separately.



SOFT CASE 9812
Includes space for small items.
Neoprene cover


CARRYING CASE 9782
Includes compartment for optional
Remote control

■ Related Products




MEMORY HILOGGER LR8400-20

30 isolated analog input channels
With built-in VOLTAGE TEMP UNIT × 2 modules



MEMORY HILOGGER LR8401-20

30 isolated analog input channels
With built-in UNIVERSAL UNIT × 2 modules



MEMORY HILOGGER LR8402-20

30 isolated analog input channels
With built-in UNIVERSAL UNIT × 1
VOLTAGE TEMP UNIT × 1 modules



MEMORY HILOGGER 8423

15 to 120 isolated analog channels, with up to
600-channel systems available
Isolated pulse input and alarm output, LAN/USB support,
for measuring with a PC



MEMORY HICORDER 8870-20

Dual-channel (isolated) high-speed oscilloscope
Measures at 1 MSa/s and displays instantaneous
AC waveforms up to 280 V
External dimensions are the same as Model LR8431-20